

[illegible]

**(43) International Publication Date**  
**19 September 2002 (19.09.2002)**

**PCT**

**(10) International Publication Number**  
**WO 02/073171 A1**

**(51) International Patent Classification<sup>7</sup>:** **G01N 21/55**

(74) Agent: **WIDÉN, Björn**; Biacore AB, Rapskatan 7, S-754 50 Uppsala (SE).

(21) International Application Number: PCT/SE02/00482

(81) **Designated States (national):** AU, CN, JP, US.

**(22) International Filing Date:** 14 March 2002 (14.03.2002)

(84) **Designated States (regional):** European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR).

(25) Filing Language: English

(26) **Publication Language:** English

**Declaration under Rule 4.17:**

— as to applicant's entitlement to apply for and be granted a patent (Rule 4.17(ii)) for the following designations AU, CN, JP, European patent (AT, BE, CH, CY, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE, TR)

(30) **Priority Data:**

0100889-5	14 March 2001 (14.03.2001)	SE
60/276.637	16 March 2001 (16.03.2001)	US

(71) Applicant (for all designated States except US): **BIA-CORE AB** [SE/SE]; Rapsegatan 7, S-751 50 Uppsala (SE).


**Published:**  
with international search report

(72) Inventor; and

(75) **Inventor/Applicant (for US only):** IVARSSON, Bengt  
[SE/SE]: Fögderivägen 22, S-740 22 Bällinge (SE).

*For two-letter codes and other abbreviations, refer to the "Guidance Notes on Codes and Abbreviations" appearing at the beginning of each regular issue of the PCT Gazette.*

(54) Title: APPARATUS AND METHOD FOR TOTAL INTERNAL REFLECTION SPECTROSCOPY

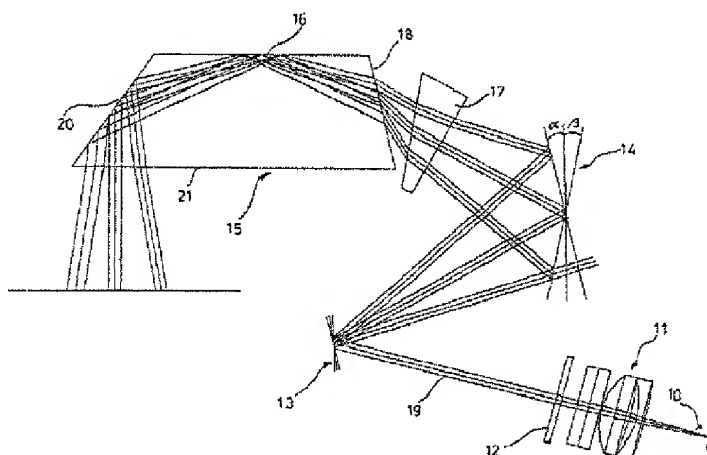

**(57) Abstract:** An optical apparatus for total internal reflection spectroscopy comprises: a transparent body (815) having an internally reflective surface (16), at least one source of electromagnetic radiation (10) for providing at least one beam of collimated electromagnetic radiation (19); optical scanning means (13, 14) for directing the beam or beams to the transparent body so that the radiation is internally reflected at the reflective surface (16), and sequentially or continuously scanning the incident angle of the radiation over an angular range; at least one detector for detecting electromagnetic radiation exiting the transparent body; and means (13, 14, 17, 18) for counteracting variation of the irradiance in the illuminated area of the surface during the angular scan, or the effect of such variation on the reflected beam or beams. An optical apparatus for examining thin layer structures on the surface for differences in respect of optical thickness and/or refractive index, and a method for total internal reflection spectroscopy are also disclosed.

WO 02/073171 A1

## APPARATUS AND METHOD FOR TOTAL INTERNAL REFLECTION SPECTROSCOPY

## Technical field of the invention

5           The present invention relates to improvements in total internal reflection (TIR) spectroscopy, and more particularly to an apparatus and method for TIR-based spectroscopic imaging with improved angular scanning, particularly attenuated total reflection (ATR) imaging spectroscopy and microscopy.

10 **Background of the invention**

Attenuated total reflection (ATR) spectroscopy, also known as internal reflection spectroscopy (IRS), originates in the observation by Newton almost two centuries ago that a propagating wave of radiation which undergoes total internal reflection (TIR) in a higher index of refraction medium in contact with a lower index of refraction medium gives rise to an evanescent field in the lower refractive index medium. It was, however, not until 1960 that this phenomenon was exploited for producing absorption spectra. Since then, numerous ATR-based applications have been developed, many of them in the biosensor field. In biosensors based on ATR, the evanescent field probes a thin layer (penetration depth about one wavelength) of sample-containing material at a solid/liquid interface, resulting in a measurable attenuation of the reflected radiation in proportion to the imaginary part of the refractive index of the thin layer, i.e. absorption spectroscopy.

As is well-known, the spectrum in ATR-spectroscopy consists of a reflectance vs. wavelength curve or spectrum, where the angle of incidence may be scanned in order to vary evanescent wave penetration depth (see e.g. Harrick, N. J., *Internal Reflection Spectroscopy*, Harrick Scientific Corp., New York, 1967; and Mirabella, F. M. Jr., *Internal Reflection Spectroscopy: Review and Supplement*, Harrick Scientific Corp., New York, 1985). Photon absorbance at the ATR-sensor surface, with or without evanescent electrical field strength enhancing metal film or particles, is detected as a more or less sharp and deep minimum, or dip, in the internal reflectance (TIR) curve, and the depth (absorbance peak) is a measure of the amount of detected sample, and the wavelength is used to identify the kind of molecule.

A variant of ATR-spectroscopy, hereinafter referred to as SPR-spectroscopy, is based on surface plasmon resonance (SPR) in an electrical field strengthening layer of metal film or metal islands or particles applied on the solid medium at the solid/liquid interface. The angle (or wavelength) corresponding to the minimum or centroid of the photon absorbance peak, or reflectance dip, and/or the change in angle, is a measure of the amount of detected sample. More particularly, the change in SPR-angle and/or SPR-wavelength is a measure of the change in the real part of the refractive index ( $n$ ) and/or the change in the thickness ( $d$ ) of the sample interaction layer or layers at the solid/liquid interface. If the sample also allows photon absorbance, this can be measured via changes in the shape (reflectance minimum and dip width) of the SPR-ATR-curve.

The surface concentration of the sample can be calculated from the shift in SPR-angle and/or SPR-wavelength by use of well-known relations between surface concentration and layer structural parameters  $n$ ,  $d$ , and empirical or calculated refractive index increment of the sample solute (De Feijter, J.A., et al., *Biopolymers* 17 (1978), 1759; and Salaman, Z., et al., *Biochemistry* 33 (1994), 13706).

In some SPR-spectroscopic optic configurations, e.g. using both p- and s-polarised light, the photon absorbance is converted into a peak rather than a dip in the reflectance curve, and the angle (or wavelength) position, or shift in position, for this peak is used as a quantitative measure of the amount, or change in amount, of detected sample.

SPR-based sensors are commercially available for use in research and development, for example the BIACORE<sup>®</sup> instrument line from Biacore AB, Uppsala, Sweden. These instruments use a sensor glass chip covered with a thin gold film and an integrated fluid cartridge for passing sample fluid and other fluids over the sensor chip. A fan shaped beam of light is coupled to the sensor chip via a prism such that an angular range of incident light is reflected internally along a line at the glass/gold film interface creating a plasmon evanescent field at the gold film/fluid interface, and the reflected light intensity distribution versus angle of incidence for a row of sensor spots along the illuminated line, is detected by a photodetector array.

The sensitivity in the detectable change of the angle (or wavelength) at the dip or peak (or in some cases, dips or peaks) of the SPR spectrum is mainly limited by the degree of constancy, drift and noise of the background light intensity of the TIR-curve. Ideally, the TIR-curve is constant versus angle. In practice, however, due to variation of

reflectance with the angle of incidence, and the radiation distribution from the light source, the TIR-curve will generally be a gaussian type curving line with at least one maximum and which at its low and high angle ends, respectively, is more or less sloping. The sensitivity of SPR-spectroscopy is, of course, particularly in the case of kinetic studies (measurement of the time dependence of the reflectance curve, shape and/or position), higher the more stable the light intensity at total internal reflection is over the angular or wavelength range of interest, i.e. the less dependent the "background" TIR-curve is on the angle (or wavelength).

The sensitivity of SPR-spectroscopy can thus be further increased if the TIR-curve is normalized, such as by a computer software algorithm. This usually requires highly stable TIR-curve data, i.e. low temporal noise and drift, and that the TIR-curve has as little curvature and sloping as possible and is as smooth as possible. Such computerized normalisation of the TIR-curve is, for example, done in the BIACORE® instruments mentioned above, where the normalisation procedure is performed on the TIR-spectrum with a sample of refractive index high enough to give TIR for the angle range used. Due to the use of a focused light beam (spot or line) and a static optical system in the present BIACORE® instruments, the illuminated sensor surface for TIR is fixed (stationary). The stability of the provided irradiance is therefore only limited by noise and drift in the light source.

Whereas conventional ATR-spectroscopy measures the surface characteristics of a sample at a fixed small spot or a thin line, spatial scanning of the incident light beam across a surface area may produce an image of the spectral property distribution over the scanned area. This technique is usually referred to as ATR-microscopy. Thus, for instance, various arrangements for surface plasmon microscopy (SPM) have been proposed for detection of the spatial distribution of the refractive index. Rather than spatially scanning a focused line or light beam across the sensor surface area with time, it has also been described to momentarily illuminate and image the whole surface area in question and scan the incident light angle or wavelength with time. A biosensor based on ATR-microscopy may, for example, be used for analyzing a large number, or an array, of sample spots simultaneously.

An example of an ATR-sensor apparatus of the last-mentioned type based on scanning the angle of incidence of a probing collimated (parallel) beam which illuminates the whole surface area is disclosed in WO 98/34098 (the full disclosure of

which is incorporated by reference herein). A representative illustration of this system is given in Fig. 1 herein, where a light source, LS, illuminates a collimator optics, CO, to produce a parallel light beam. The beam passes an interference filter, I, as a monochromatic beam and impinges on a first flat scanner mirror, SM1, to be deflected  
5 onto a second scanning mirror, SM2. The latter deflects the beam into a prism Pr for coupling the light into a sensor surface, SS, the beam being totally internally reflected at the sensor interface side of the coupling prism. The p-polarized component of the beam then passes a polarizer, P, whereupon the beam is directed into a spherical objective, SO, to produce a real image on a photo detector array or matrix, D, of the sensor surface  
10 area from its reflected light intensity pattern.

The detector array D is arranged such that the real image of the sensor area is produced on a rectangular part, D, of the array, the objective SO having its real image plane positioned at the plane of the photodetector array. Numerals 1, 2 and 3 at the detector array D denote the respective images of the corresponding subzones on the  
15 sensor surface SS, indicated at 1', 2' and 3', respectively.

The two scanning mirrors SM1 and SM2 have a related rotational or oscillating movement to produce an angularly scanned collimated beam incident within a range of angles of incidence on the sensor surface side of the prism Pr. "Beam walking" of the illuminated area, which is caused by refraction of the collimated light at the entrance of  
20 the prism Pr during the scan of the angle of entrance and would give an irregular irradiance (radiant power per unit area) at the sensor surface, is avoided by synchronizing the movements of the scanning mirrors SM1 and SM2 (as well as adapting the distances and angles between mirrors and prism, and scanned angular range of the mirrors) to provide a fixed centre for the intersection of the incident  
25 collimated light beam with the sensor surface SS.

In the general type of ATR-microscope described above, the momentary incident angle of the collimated light beam irradiating the sensor surface during the angle scan may be determined by various means. WO 98/34098 proposes to determine the momentary incident angle by detecting a part of the light beam reflected at the  
30 sensor surface on a second detector. More particularly, the objective SO comprises an additional part having its back focal plane positioned at the plane of the photodetector array to permit a minor part of the reflected collimated beam to be focused onto a

minor, linear part of the detector area so that each angle of reflection corresponds to a specific linear detector position within the detector area.

While in the ATR-microscope described in WO 98/34098 the fixed centre of the illuminated area thus gives a more stable irradiance, or optical power distribution across the cross-section of the beam at the sensor surface than in the case of beam walking, this ATR-microscope has another shortcoming.

Thus, in WO 98/34098, as in conventional ATR-spectroscopy, the centre angle of the collimated beam is orthogonally incident onto the entrance surface of the ATR-prism. During the angle scan of this collimated beam, however, the angle of incidence at the entrance surface of the prism will be oblique, a typical angle range being, say, 15°. Therefore, even for an illuminated ATR-sensor area with eliminated beam walking, i.e. a fixed centre during angle scan, there will be a variation in the light intensity, or irradiance, with the angle of incidence since the intersection area of the incident collimated beam (of mainly constant beam cross-section area) with the ATR-surface will vary in accordance to Lambert's Cosine Law. The length of the intersection area thus has a fixed centre but the length may be said to "oscillate" around its centre.

For example, if the length of the intersection area is denoted  $L$ , the length  $L = (\text{beam diameter}) / \cos(\text{angle of incidence})$ , or, in case of a rectangular beam cross section,  $L = (\text{beam cross-section length}) / \cos(\text{angle of incidence})$ . This causes, even if the beam walking has been eliminated,  $L$  (and the illuminated area) to increase, and the irradiance to decrease, the larger the angle of incidence at the sensor area. The irradiance is proportional to  $\cos(\text{angle of incidence})$ , during the angle scan by the following exemplary factors: for angle of incidence scan 63° to 77°: 2.0x; for angle of incidence scan 62° to 82°: 3.37x; and for angle of incidence scan 64° to 84°: 4.19x.

This monotone continuously decreasing light intensity with  $\cos(\text{angle of incidence})$  creates a correspondingly sloping TIR-data vs. angle curve. As is readily seen, the reflectance at 77° will be about 50 % of that at 63°, and at 84° only about 25 % of that at 63°.

Such a substantial decrease in light intensity with increased angle of incidence can not readily be compensated for by computerized data processing like the above-mentioned normalisation of the TIR-curve, or at least not without a complex normalization method and software. There is therefore a need for means which

overcome the problem of varying light intensity during angular scan in ATR-based microscopy.

Related to ATR-microscopy are other microscopic techniques also based on the evanescent wave phenomenon at total internal reflection without or with evanescent field enhancing metal films or textures, such as, for example, total internal reflection fluorescence (TIRF), total internal reflection phosphorescence, and scattered total internal reflectance (STIR). To overcome the above-mentioned problem of varying light intensity during angular scan would therefore be valuable also in those as well as in other related TIR-techniques.

10

### Summary of the invention

The present invention overcomes the disadvantages of the prior art TIR-based microscopes, such as the ATR-microscope, and offers additional advantages. In brief, the present invention is based on the concept of varying the intensity of the collimated beam incident on a TIR-sensor surface of fixed centre position (i.e. eliminated beam walking) with the angle of incidence, such that lengthwise extension of the illuminated sensor surface area as the angle of incidence is increased, or the effect of such length extension, is counteracted. In this way, the variation of the radiation intensity at the TIR-sensor surface of fixed centre position during angular scan may thus be eliminated or at least considerably reduced.

20

In one aspect, the present invention therefore provides an optical apparatus for total internal reflection (TIR) spectroscopy comprising:

a transparent body having a first entrance surface for incident electromagnetic radiation, a second plane internally reflective surface for reflecting radiation transmitted from the first surface through the transparent body, and a third exit surface through which electromagnetic radiation reflected at the second surface exits the transparent body,

25

at least one source of electromagnetic radiation,

collimating means for collimating radiation emitted from the at least one source of electromagnetic radiation to at least one beam of collimated electromagnetic radiation,

30

optical scanning means, arranged between the collimating means and the transparent body, for directing at least part of the collimated electromagnetic radiation

to the transparent body so that the radiation is internally reflected at the second surface ,  
and sequentially or continuously scanning the incident angle of the radiation at the  
second surface over an angular range, the illuminated area or areas having an at least  
substantially fixed centre position, and

- 5           at least one detector for detecting electromagnetic radiation exiting from the  
transparent body.

The apparatus is characterized in that it comprises means for varying the cross-  
sectional intensity of at least one of (i) the at least one beam of collimated  
electromagnetic radiation incident on the second plane surface of the transparent body  
10       and (ii) the at least one beam of collimated electromagnetic radiation reflected from the  
second plane surface of the transparent body, in dependence of the incident angle at the  
second surface during the angular scan, so that variation of the irradiance at the  
illuminated area or areas of fixed centre position of the second plane surface due to  
varying length extension in the plane of incidence of the illuminated area or areas  
15       during the angular scan, or the effect of such variation on the reflected beam or beams,  
is counteracted.

In one embodiment of the above-mentioned aspect of the present invention, the  
apparatus is to be used for attenuated total reflection (ATR) spectroscopy and the  
detector or detectors are arranged to detect electromagnetic radiation totally internally  
20       reflected at the second surface and exiting from the third surface of the transparent  
body.

In another embodiment, the detector or detectors are arranged to detect  
electromagnetic radiation originating from evanescent wave stimulated fluorescence or  
phosphorescence of a substance(s) in contact with the second reflective surface of the  
25       transparent body.

In still another embodiment, the detector or detectors are arranged to detect  
electromagnetic radiation originating from scattering of a substance(s) at the second  
surface of the transparent body.

In yet another embodiment, the detector or detectors are arranged to detect at  
30       least two of electromagnetic radiation totally internally reflected at the second surface,  
electromagnetic radiation originating from evanescent wave stimulated fluorescence or  
phosphorescence, and electromagnetic radiation originating from scattering at the  
second surface of the transparent body.



The above mentioned entrance and exit surfaces of the transparent body may optionally be one and the same surface.

In another aspect, the present invention provides an optical apparatus for examining thin layer structures on a surface for differences in respect of optical  
5 thickness (and/or refractive index), comprising:

a sensor unit having at least one sensing surface with a number of zones capable of exhibiting thin layer structures of varying optical thickness, particularly as the result of contact with a sample,

at least one source of electromagnetic radiation,  
10 collimating means for collimating radiation emitted from the at least one source of electromagnetic radiation to at least one beam of collimated electromagnetic radiation,

optical means for coupling at least part of the collimated electromagnetic radiation to the sensor unit to illuminate a sensing surface area or areas thereof,  
15 detector means,

means for imaging onto the detector means at least one of (i) radiation internally reflected from the illuminated sensing surface area or areas, (ii) radiation originating from sample on the sensing surface through evanescent wave stimulated fluorescence or phosphorescence, and (iii) radiation originating from scattering from sample at the  
20 sensing surface, for detecting the intensities of the radiation reflected or originating, respectively, from the different parts of the illuminated area or areas,

means for sequentially or continuously scanning the radiation incident at the optical coupling means and at the illuminated area or areas of the at least one sensing surface over a range of incident angles, the illuminated area or areas having an at least  
25 substantially fixed centre position,

means for determining each angle of incidence of electromagnetic radiation impinging on the at least one sensing surface, and

evaluation means for determining from the relationship between detected intensity of radiation imaged on the detector means and incident angle of the radiation  
30 reflected at the sensing surface or surfaces, the optical thickness of each sensing surface zone to thereby produce a (morphometric) image of the optical thickness of the at least one sensing surface.

The apparatus is characterized in that it comprises means for varying the cross-sectional intensity of at least one of (i) the at least one beam of collimated electromagnetic radiation incident on the at least one sensing surface area of the sensor unit, and (ii) the at least one beam of collimated electromagnetic radiation reflected from the at least one sensing surface area, in dependence of the incident angle at the sensing surface or surfaces during the angular scan, so that the variation of the irradiance in the illuminated area or areas of fixed center position of the sensing surface or surfaces due to varying length extension in the plane of incidence of the illuminated area or areas during the angular scan, or the effect of such variation on the reflected beam or beams, is counteracted.

In still another aspect, the present invention provides a method of performing total internal reflection based spectroscopy, which method comprises:

irradiating at least one area of a plane surface of a transparent body with at least one collimated beam of electromagnetic radiation so that the radiation is totally internally reflected at the surface,

imaging onto a respective two-dimensional detector array at least one of (i) radiation internally reflected from the illuminated area or areas, (ii) fluorescent or phosphorescent radiation from the illuminated area or areas caused by evanescent wave stimulation, and (iii) radiation originating from evanescent wave stimulated scattering at the illuminated area or areas,

sequentially or continuously scanning the incident angle over an angular range, the illuminated area or areas having an at least substantially fixed centre position during angular scan,

measuring at at least a number of incident angles of the radiation reflected at the plane surface of the transparent body, the intensities of the radiation imaged on different parts of the detector array (D), and

determining from the detected radiation intensities at the different incident angles at the transparent body surface, at least one of an optical thickness image, a refractive index image, a surface concentration image of the surface, and the variation of such images with time.

The method is characterized in that it comprises continuously varying the cross-sectional intensity of at least one of (i) the at least one beam of collimated electromagnetic radiation incident on the plane surface of the transparent body, and (ii)

the at least one beam of collimated electromagnetic radiation reflected from the plane surface of the transparent body, in dependence of the incident angle at the surface during the angular scan to reduce variations of the intensity of radiation in the illuminated area or areas of fixed centre position of the surface due to varying length extension in the plane of incidence of the illuminated surface area or areas of fixed centre position during the angular scan, or the effect of such variation with time on the reflected beam or beams.

In one embodiment, the method is used for kinetic studies of binding events at a sensor surface.

In a particular embodiment of the above method aspect of the invention, ATR-spectroscopy is performed, i.e. the radiation internally reflected from the illuminated area or areas is imaged onto the detector array.

In preferred embodiments of the above apparatus and method aspects of the invention, variations of the intensity of radiation in the illuminated area(s) of the surface of the transparent body caused by varying length extension of the illuminated area(s) during the angular scan are counteracted by varying the length extension in the plane of incidence of the incident beam (or beams) of collimated electromagnetic radiation in dependence of the incident angle during the angular scan, and more particularly such that the beam cross sectional area is decreased as the angle of incidence at the surface is increased.

Optionally, the apparatuses and method, respectively, of the present invention are arranged to permit use of at least two different wavelengths.

The above and other aspects of the invention will be evident upon reference to the attached drawings and the following detailed description.

#### Brief description of the drawings

Fig. 1 is a schematic sectional view of a prior art ATR-microscopy system.

Fig. 2 is a schematic sectional view of an embodiment of apparatus according to the present invention.

Fig. 3 is a diagram showing total internal reflectance (TIR) versus incident angle for (A) the apparatus of Fig. 2, and (B) a prior art ATR-sensor with fixed centre during angle scan.

Fig. 4 is a schematic sectional view of another embodiment of apparatus according to the present invention.

Fig. 5 is a diagram showing total internal reflectance (TIR) versus incident angle during angle scan for the apparatus of Fig. 4.

5

### Detailed description of the invention

As mentioned above, the present invention is directed to overcoming in TIR-based microscopy, such as ATR-microscopy, the problem of varying irradiance at an internally reflective surface, such as that of an ATR-prism, when irradiating the surface with collimated electromagnetic radiation (with or without beam-walking) and scanning the angle of incidence over an angular range. As already set out, the variation in irradiance is due to the beam intersection increasing as the angle of incidence increases at the beam-intersected internally reflective surface.

According to the invention, this problem is solved by providing means for counteracting the undesired variation in radiation intensity at the internally reflective surface with the angle of incidence to provide for a substantially constant radiation intensity of the incident collimated beam in the plane of the internally reflective surface during the angle scan, or, alternatively, counteracting the effect of such variation on the reflected beam. This may be achieved by either (i) for a beam of constant optical power, continually decreasing the cross-section dimension of the beam (or beam diameter for a circular beam) incident at the internally reflective surface as the angle of incidence at the reflective surface is increased; (ii) for a beam of variable optical power, continually increasing the intensity of the (incident or reflected) beam of electromagnetic radiation as the angle of incidence at the reflective surface is increased; or (iii) using a combination of variants (i) and (ii).

25

It is also within the scope of the present invention to reduce the effect of such undesired variation of the irradiance at the reflective surface by affecting or modifying the detector response, such as, e.g., modifying the response signal from the detector, optionally in combination with one or more of the approaches (i) and (ii) above.

30

Some of the technical terms and expressions used in this specification and the appended claims will be defined below or are as defined in the above-mentioned WO 98/34098 (the disclosure of which is incorporated herein by reference in its entirety).

Otherwise, the technical terms and expressions have the same meaning as commonly understood to one of ordinary skill in the art to which this invention belongs.

The term "electromagnetic radiation" as used herein means radiation in the visible region (from about 400 to about 750 nm) and in the infrared region (from about  
5 750 nm to about 20  $\mu\text{m}$ ), i.e. in the wavelength range from about 0.4  $\mu\text{m}$  to about 20  $\mu\text{m}$ . For simplicity, it will in the following description be referred to as "light".

The "source of electromagnetic radiation" may, for example, be a light emitting diode (LED), laser diode, or an array or bar of LED's or laser diodes. For simplicity, it will hereinafter be referred to as "light source".

10 The "transparent body" may be an integral element or consist of two (or optionally more) separate elements in optical light-coupling contact with each other. The transparent body containing the internally reflective surface will below often be referred to as transparent ATR-body, or simply ATR-body or ATR-prism, and for simplicity also in total internal reflection contexts not restricted to ATR.

15 The term "optical thickness" as used herein defines a composite optical property of a material which is a function of both its physical thickness and its refractive index (the complex index of refraction ( $\tilde{n}$ ) consists of a real part ( $n$ ) responsible for beam refraction, and an imaginary part ( $k$ ) responsible for the absorption, or beam attenuation, in the medium, i.e.  $\tilde{n} = n - ik$ ).

20 Morphometric images of the optical thickness, as obtainable by the present invention, may reflect a change in refractive index and/or physical thickness.

The internally reflective surface supports the thin layer of matter to be probed by the evanescent wave elicited by total internal reflection (such as in ATR) and will below often be referred to as a sensor surface.

25 As is well known, there are two common ways of coupling the light to the sensor surface for creation of an evanescent wave, either by a prism or by a grating. As is also well known, in the prism-coupling case, the sensor surface may be a surface of the prism or that of a separate sensor element, such as a glass or plastic plate, in optical light-coupling contact with the prism, such as via a refractive index matching medium.  
30 In the latter case, the "internally reflective surface" will be a surface of this separate sensor element. In the grating-coupling case, the sensor surface may be integral with the grating element, e.g. be one face of a glass or plastic plate with the grating formed on

the opposite face or be a part of the grating. As in the prism case, the sensor element may also be a separate element in optical contact with a grating element.

The sensor element may alternatively be integral with a surface providing optical coupling via refraction or diffraction, such as, for example, be one face of a glass or plastic plate with micro-prisms or Fresnel lenses formed on the opposite face, e.g. as described in WO 92/05426 (the entire disclosure of which is incorporated by reference herein).

With reference to variant (i) above, controlled variation of the beam cross-section may be obtained by "oblique incidence" of the beam at the entrance surface of an ATR-body. By "oblique incidence" is meant that the angle scan only includes angles on one and the same side of the normal to the entrance surface. In this way, the diameter in the plane of incidence of the beam passing through the prism onto the sensor surface will vary during the angle scan so that it is largest for the smallest angle of incidence at the internally reflective surface of the ATR-body, and smallest for the largest angle of incidence, thereby giving a reduced variation of the illuminated area and reducing the dependence of the length of the illuminated area on the sensor surface with the angle of incidence.

While the oblique incidence at the ATR-body, on the one hand, thus will provide for an at least substantially reduced variation of the irradiance of the illuminated area of the sensor surface, such oblique incidence may, on the other hand, give rise to beam walking (as defined above).

For scanner mirrors with symmetric scan mirror angle-amplitudes used with oblique incidence to minimise variation of irradiance, beam walking may be avoided by having the collimated beam pass of a wedge shaped transparent body before reaching the ATR-body to thereby obtain a fixed illuminated area centre.

An orthogonal incidence of the beam at the entrance surface of the ATR-body, as in the prior art system disclosed in the above-mentioned WO 98/34098, and symmetric scan mirror amplitudes also provides a symmetric angle of incidence range (i.e. symmetric angle of incidence amplitude around the centre angle of incidence corresponding to the centre angles of the scanner mirrors), e.g.  $70.0 \pm 6.0^\circ$ . However, in an optical design based on "oblique incidence" of the beam at the entrance surface of the ATR-body, and a wedge-shaped transparent body to eliminate beam walking, the

angle of incidence amplitudes will be non-symmetric, e.g. ranging from  $70.0 + 7.0^\circ$  to  $70.0 - 6.0^\circ$ .

Alternatively, beam walking of the collimated beam caused by the irradiation variation minimising the oblique incidence surface on the ATR-body may be eliminated  
5 by using asymmetric scan-mirror angle amplitudes, the asymmetry of the scan-mirror amplitudes providing the desired fixed illuminated area centre.

In one embodiment, the scanner mirrors comprise first and second oscillating mirrors, the angle scan amplitudes of which are symmetrical around the centre angle of the scanning, which centre angle corresponds to the operational centre angle of  
10 incidence range of the collimated beam. Preferably, the scan angle amplitude ratio of the second oscillating mirror to that of the first oscillating mirror is from about 1 to about 10.

In another embodiment, the scanner mirrors comprise first and second rotating mirrors. Preferably, the scan angle amplitude ratio of the second rotating mirror to that  
15 of the first rotating mirror is from about 1 to about 10.

As to variant (ii) above, the power of the light beam produced by the light source, i.e. the light output, may be controlled by regulating the drive current/voltage of the light source, and more particularly to increase the drive current/voltage as the angle of incidence at the sensor surface is increased. Alternatively, the light beam may be  
20 caused to pass an electromechanical beam intensity attenuator, such as a filter means having an electronically controlled variable attenuating effect on the light intensity of the beam, e.g. a linear polariser rotated in relation to a following p-polariser, or variable neutral density filters. Such filter means may be arranged in the path of either (or possibly both of) the incident or the reflected light beam, preferably before the incident  
25 light beam is reflected by the scanning means. When regulating the light source drive current or voltage, or the drive current or voltage for the beam intensity attenuator, a control signal from the photodetector, where the control signal is proportional to the detected irradiance on the detector, can be used in the regulating process.

According to variant (iii) mentioned above, a combination of variants (i) and (ii)  
30 may be used. For example, it may be found convenient to use variant (i) for a first range of incident angles, and variant (ii) for a second range of incident angles.

While usually a single light source (e.g. a light emitting diode, or a laser diode) together with a lens system is used to create the collimated beam, the use of a plurality

of light sources may also be contemplated to create a plurality of collimated beams to be scanned in parallel by the scanning means. In this way, a plurality of parallel sensor surfaces may be illuminated and sensed. It is, of course, also possible to use two or more light sources to create a combined single beam. These light sources may have  
5 identical wavelength or different wavelengths.

As already mentioned, the inventive concept of the present invention as described above, is also applicable to other TIR-based technologies than ATR-spectroscopy. Thus, for instance, rather than measuring the intensity of a totally internally reflected beam of light, fluorescence or phosphorescence emitted from a  
10 sensing surface due to excitation by evanescent wave resulting from the total internal reflection may be measured versus angle of incidence. Such fluorescence or phosphorescence may be emitted from either natively fluorescent or phosphorescent sample molecules or molecules labelled with a fluorophore or phosphorophore. Total internal reflection fluorescence is commonly referred to as TIRF.

15 In SPR-TIRF or SPR-total internal reflection phosphorescence, an SPR-field is used to stimulate the emission of fluorescence or phosphorescence.

Alternatively, light originating from evanescent wave excited scattering at the sensing surface may be measured versus angle of incidence. This technology is usually referred to as STIR (scattered total internal reflection).

20 The use of TIRF, total internal reflection phosphorescence and STIR, respectively, is described in, for example, US-A-5,313,264.

It is also possible to use any one of the above non-ATR techniques in combination with ATR, i.e. in combination with measuring the intensity of a totally internally reflected light beam.

25 US-A-6,194,223, for example, discloses a method for detecting an analyte, wherein a first signal from SPR-measurement and a second signal from fluorescence measurement are independently analysed.

WO 98/22808 discloses an SPR apparatus comprising a first detector for detecting light internally reflected from a sensor surface, and a second detector for  
30 detecting light scattered or emitted from an analyte bound at the sensor surface.

The entire disclosures of the three patent publications mentioned above are incorporated by reference herein.



In the following the invention will be described, by way of example only, with regard to some specific embodiments thereof.

The invention may advantageously be applied to a TIR-based optical system of the general type disclosed in the above-mentioned WO 98/34098 and schematically illustrated in Fig. 1 as briefly described above. Fig. 2 discloses a modification according to the present invention of a part of the prior art system illustrated in Fig. 1. Like the system in Fig. 1, the inventive embodiment of Fig. 2 comprises a light source 10, e.g. a light emitting diode (LED), collimator optics 11, an interference filter 12, a pair of scanning mirrors, namely a first scanning mirror 13 and a second scanning mirror 14, and an ATR-prism 15 with a sensor surface 16. The two scanning mirrors 13 and 14 are arranged to have symmetric scan-mirror angle amplitudes as is shown in Fig. 2 ( $\alpha = \beta$ ). Such scanning mirrors are well known in the art, and exemplary systems are described in the above-mentioned WO 98/34098.

The sensor surface 16 may, as is well known in the art, be applied directly on the prism 15 or be provided on a separate element, as described in, for example, EP-B-442922, which element is light-coupled to the prism via an immersion oil or a so-called optointerface as described in, for example, US-A-5,164,589. The sensor surface *per se* may be any of a variety of sensor surfaces and will not be described herein any further. Suffice it to say that exemplary sensor surfaces are described in US-A-5,242,828 and US-A-5,436,161. (The disclosures of the above-mentioned U.S. and European patents are incorporated by reference herein).

In contrast to the prior art system, the optical system of Fig. 2 additionally comprises a wedge-shaped prism 17 inserted between the second scanning mirror 14 and the ATR-prism 15. Also, in the embodiment in Fig. 2, the entrance surface 18 on the ATR-prism 15 for the incident light is inclined in relation to the incident light beam such that the angle of incidence will be oblique over the whole scanned angular range as will be described below.

A beam of collimated light 19 from the light source 10 and collimated optics 11 is reflected by the scanning mirrors 13, 14 via wedge prism 17 into prism 15 where the beam is totally internally reflected at the sensor surface 16. The reflected light is then, in the illustrated case, totally internally reflected at plane prism side 20 to leave the prism through plane prism side 21 parallel to the sensor surface. The reflected light may then, in the same way as in Fig. 1 (but not shown in Fig. 2), pass a polariser and an objective

to produce an image on a detector array. For further details on the beam path components following after the prism 15, as well as on the light source and collimator optics, it is referred to the above-mentioned WO 98/34098. It may be noted that it is advantageous to focus part of the light reflected at an area of the sensor surface without sensing function, and/or light reflected at the coupling prism onto a separate part of the detector array or separate detector to determine the momentary incident angle (or wavelength).

In Fig. 2, the collimated beam enters the prism 15 with an oblique incidence angle, which means that all beams during the angle scan impinge on the prism obliquely or, expressed in another way, are all on one and the same side of the normal to the inclined entrance side 18 of prism 15, as opposed to the situation in the prior art system in Fig. 1, where the centre beam impinges orthogonally to the entrance side of the prism.

The oblique incidence in Fig. 2 causes, as is readily appreciated, the length of the intersection area of the beam with the inclined prism entrance surface 18 (length  $L = [\text{beam diameter}(\text{angle})]/\cos(\text{angle})$ ) to be continually decreased as the angle of incidence at the sensor surface 16 is increased, and thereby the length of the illuminated sensor surface area of fixed centre position, is kept mainly constant. In other words, the width of the beam incident at the sensor surface 16 (in the plane of incidence) will vary during the angle scan so that it is largest for the smallest angle of incidence at the sensor surface and smallest for the largest angle of incidence at the sensor surface. The oblique beam entrance into the prism will thus counteract the dependence of the length of the intersection area (and thereby the illuminated sensor surface area) on the  $\cos(\text{angle})^{-1}$  and provide a substantially constant illuminated area and irradiance on the sensor surface during the angle scan.

It is appreciated that when using scan mirrors with symmetric scan angle amplitudes as illustrated in Fig. 2 in combination with an oblique beam entrance onto the ATR-prism to maintain a substantially constant beam intersection area with the sensor surface according to the present invention, the oblique beam incidence may cause beam walking, i.e. a moving centre of the illuminated area. This is, however, obviated by wedge prism 17 which has a geometry and position selected to counteract the asymmetry in the angle scan caused by the oblique beam entrance into the prism and produce a symmetric angle scan. The appropriate wedge geometry, including angle of

entrance, thickness and angle of exit, to obtain such a fixed illuminated area centre and eliminate beam walking may readily be selected by the skilled person in each particular situation, bearing in mind that the use of wedge prisms (anamorphic prisms) in optical systems is *per se* known in the prior art.

5 For instance, beam shaping based on anamorphic prisms is described in, for example, O'shea, Donald C., "Elements of Modern Optical Design", Wiley & Sons, Inc. 1985, pages 259-262; and Marshall, Gerald F., "Laser Beam Scanning", Marcel Dekker, Inc. 1985, pages 346-349. A prism couple is mounted in a fixed (non-scanned) collimated beam with the purpose of obtaining a collimated beam of new cross-section  
10 ratio, the changed beam also being fixed and parallel with the first beam. An example hereof is the transformation of the elliptical output of a diode laser into a circular beam, such as e.g. in commercial collimation laser pens.

Also, beam scanning based on wedge prisms is described in Marshall, Gerald F., "Scanning Devices and Systems", Applied Optics and Optical Engineering vol. vi,  
15 Academic Press Inc, 1980, pages 248-250. A collimated beam incident onto a prism is rotated about an axis collinear with the incident beam for the purpose of refracting this beam and creating a spatial cone in space formed by the swept refracted emergent collimated beam. Further, it is described how, by the same principle, two wedge prisms contra-rotating in tandem can be used to create an elliptical cone of a swept beam  
20 position on a screen. (The entire contents of the above two publications are incorporated by reference herein.)

A main advantage of symmetric mirror scan angle-amplitudes is the resulting approximately identical angle of incidence vs. time relationship, which provides a distribution of measured angle(time)-data symmetrical around the scan angle centre,  
25 which in turn improves the speed and accuracy of the computed SPR-angle vs. time data. Another advantage of symmetric scan angle-amplitudes is a less complex driver electronics for the two synchronised mirror scanners as well as less wear of the scanner bearing design, i.e. less torsional stress, due to a symmetrical torsional (turning) moment.

30 Fig. 3 shows the variation of the reflectance versus incident angle for an optical set-up according to Fig. 2 (curve A) as compared with that for a prior art set-up with orthogonal incidence and symmetric scan angle amplitudes (curve B). As demonstrated by Fig. 3, the embodiment of Fig. 2 causes the dependence of the reflectance on the

incident angle to have a maximum reflectance within a more or less symmetrical curve shape (A) rather than the monotone sloping curve (B) obtained in the prior art. It is appreciated by the skilled person that by the use of a suitable computer software algorithm, measurement data obtained with the apparatus in Fig. 2 may be adjusted for this substantially reduced and controlled variation of the reflectance during the angle scan.

As mentioned above, computer software algorithms have been used in the prior art to normalize the TIR curve in SPR biosensor instruments. For the commercial BIACORE<sup>®</sup> instruments referred to above (i.e. static optical configuration), such a normalisation procedure includes:

- a) Filtering of measured reflectance data vs. time at each angle within the simultaneous angle of incidence range in order to obtain a continuous TIR-data curve (total reflectance vs. angle curve or plot). Such averaging over time of the detector response signal reduces the temporal scatter/noise in the TIR-data. The less scattered data, the faster is the filtering data processing (calculations) thereof into a curve smooth enough for high accuracy detection of dips and peaks.
- b) Curve fitting an analytical curve to the filtered TIR-curve. The less complex curve shape, the faster, less complex, and more accurate curve fitting data processing (calculation).
- c) Normalisation, calculation of correction data for the analytical TIR-data curve fit. The normalisation-correction data-matrix is stored in a computer memory, and is added to the analytical TIR-data curve to provide a normalised analytical TIR-data (as constant total internal reflectance as possible as function of angle of incidence).

When the sample is added and bound to the SPR-sensor surface, it causes a minimum in the measured TIR-curve, the resonance curve. The resonance curve's reflectance data are filtered in real-time and the normalisation-data matrix is added. In a real-time computer process, an analytical curve is fitted to this normalised SPR-curve, and the curve's angular position is calculated in real-time. A normalised TIR-curve improves the measurement accuracy of the angle position of the SPR- reflectance dip (or converted to reflectance peak). If no normalisation is done, the slope and low spatial frequency scatter/noise in the TIR-data will disturb the curve-shape of the SPR-curve and limit the accuracy of measured absolute and changes in SPR-curve shape

parameters (reflectance minimum/minima, reflectance peak/peaks, curve-dip/peak width) or SPR-angles, and of SPR-angle vs. time kinetic measurements.

It is appreciated that such software may be improved to also adjust for the variation of the reflectance during the angle scan as obtained with the embodiment in  
5 Fig. 2.

An alternative embodiment of the present invention is shown in Fig. 4. Like the embodiment in Fig. 2, it comprises a light source 30, collimator optics 31, an interference filter 32, a first scanning mirror 33, a second scanning mirror 34, and an ATR-prism 35 with a sensing surface 36. Also, in conformity with the embodiment in  
10 Fig. 2, a collimated light beam 37 from the light source 30 and collimator optics 31 is reflected by the scanning mirrors 33, 34 to impinge at an oblique incident angle at the entrance surface 38 of the prism 35 to thereby counteract variation of the illuminated area of the sensor surface 36 during the angle scan.

In the embodiment of Fig. 4, however, in order to eliminate beam walking, a  
15 fixed illuminated area centre is ensured by the scan-mirror angle amplitudes being asymmetric (as indicated in the Figure:  $\alpha \neq \beta$ ) in a way that counteracts the asymmetry caused by the oblique incidence at the ATR-prism. This asymmetry of the scan-mirror angle amplitudes thus replaces the wedge prism 17 in Fig. 2. Techniques for asymmetric scan-mirror angle amplitudes are known *per se* in the art.

As in the embodiment of Fig. 2, the beam totally reflected at the sensing surface  
20 36 is then reflected at plane prism side 39 and exits the prism 35 through prism side 40 to be imaged on a detector array.

The TIR-curve obtained with the embodiment in Fig. 4 is illustrated by the diagram of Fig. 5. In the same way as for the TIR-curve obtained for the embodiment in  
25 Fig. 4, the TIR-curve in Fig. 5 may be normalised by a suitable computer software algorithm.

From the foregoing, it will be appreciated that, although specific embodiments of this invention have been described herein for purposes of illustration, various modifications may be made without departing from the spirit and scope of invention.  
30 Accordingly, the invention is not limited except by the appended claims.

## Claims

1. An optical apparatus for total internal reflection (TIR) spectroscopy comprising:  
a transparent body (15; 35) having a first entrance surface (18; 38) for incident  
5 electromagnetic radiation (19; 37), a second plane internally reflective surface (16; 36)  
for reflecting radiation transmitted from the first surface through the transparent body,  
and a third exit surface (21; 40) through which electromagnetic radiation reflected at the  
second surface exits the transparent body,  
at least one source of electromagnetic radiation (10; 30),  
10 collimating means (11; 31) for collimating radiation emitted from the at least  
one source of electromagnetic radiation to at least one beam of collimated  
electromagnetic radiation (19; 37),  
optical scanning means (13, 14; 33, 34), arranged between the collimating  
means (11; 31) and the transparent body (15; 35), for directing at least part of the  
15 collimated electromagnetic radiation (19; 37) to the transparent body so that the  
radiation is internally reflected at the second surface (16; 36), and sequentially or  
continuously scanning the incident angle of the radiation at the second surface over an  
angular range, the illuminated area or areas having an at least substantially fixed centre  
position, and  
20 at least one detector (D) for detecting electromagnetic radiation exiting from the  
transparent body (15; 35),  
characterized in that the apparatus further comprises:  
means (13, 14, 17, 18; 33, 34, 38) for varying the cross-sectional intensity of at  
least one of (i) the at least one beam of collimated electromagnetic radiation (19; 37)  
25 incident on the second plane surface of the transparent body (15; 35), and (ii) the at least  
one beam of collimated electromagnetic radiation reflected from the second plane  
surface of the transparent body (15; 35), in dependence of the incident angle at the  
second surface (16; 36) during the angular scan, so that the variation of the irradiance at  
the illuminated area or areas of fixed centre position of the second plane surface due to  
30 a varying length extension in the plane of incidence of the illuminated area or areas  
during the angular scan, or the effect of such variation on the reflected beam or beams,  
is counteracted.

2. The apparatus of claim 1, **characterized** in that the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation (19; 37) incident on the second plane surface of the transparent body (15; 35) is varied.
- 5 3. The apparatus of claim 2, **characterized** in that the means for varying the cross-sectional intensity of the beam of collimated electromagnetic radiation comprise means for varying the cross-sectional area's length of the at least one beam of collimated electromagnetic radiation (19; 37) in the plane of incidence at the second plane surface (16; 36) of the transparent body (15; 35) in dependence of the incident angle during the  
10 angular scan.
4. The apparatus of claim 3, **characterized** in that the first surface (18; 38) of the transparent body is plane and that the means for varying the cross-sectional area's length of the at least one beam of collimated electromagnetic radiation comprise means  
15 for directing the beam or beams (19; 37) at an oblique angle of incidence onto the first surface such that the angle of incidence onto the first surface is continuously decreased as the angle of incidence at the second internally reflective surface (16; 36) is increased.
5. The apparatus of any one of claims 1 to 4, **characterized** in that the angle scan  
20 amplitudes provided by the optical scanning means are symmetrical around the centre angle of scanning.
6. The apparatus of claim 5, **characterized** in that a plane-sided wedge-shaped body (17) is arranged between the optical scanning means and the transparent body and  
25 fixed with regard to the transparent body.
7. The apparatus of claim 6, **characterized** in that the wedge-shaped body is a plane-sided prism (17).
- 30 8. The apparatus of any one of claims 1 to 7, **characterized** in that the scanning means comprise first and second oscillating mirrors (13, 14; 33, 34).

9. The apparatus of claim 8, **characterized** in that the ratio of the scan angle amplitude of the second oscillating mirror to that of the first oscillating mirror is from about 1 to about 10.
- 5 10. The apparatus of any one of claims 1 to 7, **characterized** in that the scanning means comprise first and second rotating mirrors.
11. The apparatus of claim 10, **characterized** in that the ratio of the scan angle amplitude of the second rotating mirror to that of the first rotating mirror is from about  
10 1 to about 10.
12. The apparatus of any one of claims 1 to 4, **characterized** in that the angle scan amplitudes provided by the optical scanning means are asymmetrical around the centre angle of scanning.
- 15 13. The apparatus of claim 12, **characterized** in that the scanning means comprise first and second oscillating mirrors (13, 14; 33, 34).
14. The apparatus of claim 13, **characterized** in that the ratio of the scan angle  
20 amplitude of the second oscillating mirror to that of the first oscillating mirror is from about 1 to about 10.
15. The apparatus of claim 12, **characterized** in that the scanning means comprise first and second rotating mirrors.
- 25 16. The apparatus of claim 15, **characterized** in that the ratio of the scan angle amplitude of the second rotating mirror to that of the first rotating mirror is from about 1 to about 10.
- 30 17. The apparatus of any one of claims 1 to 4, **characterized** in that the scanning means comprise first and second oscillating mirrors (13, 14), the angle scan amplitudes of which are symmetrical around the centre angle of the scanning, which centre angle of scanning corresponds to the centre of the operational angle of incidence range of the



collimated beam (19), and that a plane-sided wedge-shaped body, preferably a prism (17), is arranged between the optical scanning means (13, 14) and the transparent body (15) and fixed with regard to the transparent body.

5 18. The apparatus of claim 1 or 2, **characterized** in that the means for varying the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation incident at or reflected from the second plane surface of the transparent body comprise means for varying the radiation power of the incident or reflected beam.

10 19. The apparatus of claim 18, **characterized** in that the radiation power of the beam is varied before the beam is reflected by the scanning means.

20. The apparatus of claim 19, **characterized** in that the means for varying the radiation power of the at least one beam of collimated electromagnetic radiation  
15 comprise means for regulating the drive current or voltage of the at least one source of electromagnetic radiation.

21. The apparatus of claim 20, **characterized** in that the means for regulating the drive current or voltage of the at least one source of electromagnetic radiation comprises  
20 a control signal proportional to the detected intensity of the at least one beam on the detector.

22. The apparatus of claim 18 or 19, **characterized** in that the means for varying the power of the at least one beam of collimated electromagnetic radiation comprise an  
25 electro-mechanical beam power attenuator.

23. The apparatus of claim 22, **characterized** in that the electro-mechanical beam power attenuator is selected from co-operating linear polarisers and variable density filters.

30

24. The apparatus of any one of claims 18-23, **characterized** in that the apparatus comprises, in addition to the means for varying the electromagnetic radiation power of the beam, means for varying the cross-sectional area's length of the at least one beam of

collimated electromagnetic radiation in the plane of incidence at the second plane surface of the transparent body in dependence of the incident angle during angular scan.

25. The apparatus of claim 24, **characterized** in that the means for varying the cross-sectional area's length of the at least one beam of collimated electromagnetic radiation are as defined in any one of claims 4 to 18.

26. The apparatus of claim 24 or 25, **characterized** in that the means for varying the cross-sectional intensity of the beam of collimated electromagnetic radiation comprise, for a first range of angle scan, means for varying the cross-sectional area of the at least one beam of collimated electromagnetic radiation in the plane of incidence at the second plane surface of the transparent body, and for a second range of angle scan, means for varying the radiation power of the at least one beam of collimated electromagnetic radiation, preferably before the beam is reflected by the scanning means.

27. The apparatus of any one of claims 1 to 26, **characterized** in that the transparent body is a plane-sided prism (15; 35).

28. The apparatus of any one of claims 1 to 27 for attenuated total reflection (ATR) spectroscopy, **characterized** in that the detector or detectors (D) are arranged to detect electromagnetic radiation totally internally reflected at the second surface (16; 36) and exiting from the third surface (21; 40) of the transparent body (15; 35).

29. The apparatus of any one of claims 1 to 27, **characterized** in that the detector or detectors are arranged to detect electromagnetic radiation originating from evanescent wave stimulated fluorescence or phosphorescence of a substance or substances in contact with the second surface of the transparent body.

30. The apparatus of any one of claims 1 to 27, **characterized** in that the detector or detectors are arranged to detect electromagnetic radiation originating from scattering at the second surface of the transparent body.

31. The apparatus of any one of claims 1 to 27, **characterized** in that the detector or detectors are arranged to detect at least two of electromagnetic radiation totally internally reflected at the second surface, electromagnetic radiation originating from evanescent wave stimulated fluorescence or phosphorescence, and electromagnetic radiation originating from scattering at the second surface of the transparent body.

32. An optical apparatus for examining thin layer structures on a surface for differences in respect of optical thickness, comprising:

a sensor unit having at least one sensing surface (16; 36) with a number of zones capable of exhibiting thin layer structures of varying optical thickness, particularly as the result of contact with a sample,

at least one source of electromagnetic radiation (10; 30),

collimating means (11; 31) for collimating radiation emitted from the at least one source of electromagnetic radiation to at least one collimated beam of electromagnetic radiation (19; 37),

optical means for coupling at least part of the electromagnetic radiation to the sensor unit to illuminate a sensing surface area or areas thereof,

first detector means (D),

means for imaging onto the first detector means (D) at least one of (i) radiation internally reflected from the illuminated sensing surface area or areas, (ii) radiation originating from sample on the sensing surface through evanescent wave stimulated fluorescence or phosphorescence, and (iii) radiation originating from scattering from sample at the sensing surface, for detecting the intensities of the radiation reflected or originating, respectively, from the different parts of the illuminated area or areas,

means (13, 14; 33, 34) for sequentially or continuously scanning the radiation incident at the optical coupling means and at the illuminated area or areas of the at least one sensing surface (16; 36) over a range of incident angles, the illuminated area or areas having an at least substantially fixed centre position,

means for determining each angle of incidence of electromagnetic radiation impinging on the at least one sensing surface (16; 36), and

evaluation means for determining from the relationship between detected intensity of radiation imaged on the first detector means and incident angle of the radiation reflected at the sensing surface or surfaces, the optical thickness of each

sensing surface zone to thereby produce an image of the optical thickness of the at least one sensing surface,

**characterized** in that the apparatus comprises:

means (13, 14, 17, 18; 33, 34, 38) for varying the cross-sectional intensity of at least one of (i) the at least one beam of collimated electromagnetic radiation (19; 37) incident on the at least one sensing surface area (16; 36) of the sensor unit, and (ii) the at least one beam of collimated electromagnetic radiation (19; 37) reflected from the at least one sensing surface area (16; 36), in dependence of the incident angle at the sensing surface or surfaces during the angular scan, so that the variation of the irradiance in the illuminated area or areas of fixed centre position of the sensing surface or surfaces due to a varying length extension in the plane of incidence of the illuminated area or areas during the angular scan, or the effect of such variation on the reflected beam or beams, is counteracted.

33. The apparatus of claim 32, **characterized** in that the apparatus comprises means for varying the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation (19; 37) incident on the at least one sensing surface (16; 36).

34. The apparatus of claim 32 or 33, **characterized** in that the means for varying the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation comprise means for varying the cross-sectional area's length of the at least one beam of collimated electromagnetic radiation (19; 37) in the plane of incidence at the at least one sensing surface in dependence of the incident angle during the angular scan.

35. The apparatus of claim 32 or 33, **characterized** in that the means for varying the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation incident at or reflected from the sensing surface or surfaces comprise means for varying the radiation power of the beam.

36. The apparatus of claim 35, **characterized** in that the radiation power of the beam is varied before the beam is reflected by the scanning means.

37. The apparatus of claim 36, **characterized** in that the means for varying the power of the at least one beam of collimated electromagnetic radiation comprise means for regulating the drive current or voltage of the at least one source of electromagnetic radiation.

5

38. The apparatus of claim 37, **characterized** in that the means for regulating the drive current or voltage of the at least one source of electromagnetic radiation comprise a control signal derived from a detector exposed to at least a part of the at least one beam reflected at the sensing surface area or areas, optionally at a sensing surface area or areas without sensing function.

10

39. The apparatus of any one of claims 32 to 38, **characterized** in that the apparatus comprises means for focusing a part of the electromagnetic radiation reflected at at least one of the coupling means and a sensing surface area without sensing function onto a second detector means, wherein each position of the focused radiation is related to a specific angle and/or wavelength of the radiation incident at the at least one sensing surface.

15

40. The apparatus of any one of claims 32 to 39, **characterized** in that the sensing surface or surfaces comprise a layer of a metal supporting surface plasmon resonance (SPR).

20

41. The apparatus of any one of claims 32 to 40, **characterized** in that the first detector means (D) detect radiation internally reflected from the illuminated sensing surface area or areas.

25

42. The apparatus of any one of claims 32 to 40, **characterized** in the first detector means detect radiation originating from evanescent wave stimulated fluorescence, particularly SPR-excited fluorescence.

30

43. The apparatus of claim 41, **characterized** in the apparatus further comprises third detector means arranged to detect radiation originating from evanescent wave stimulated fluorescence, particularly SPR-excited fluorescence.

44. The apparatus of claim 41, **characterized** in the apparatus further comprises third detector means arranged to detect radiation originating from evanescent wave stimulated phosphorescence, particularly SPR-excited phosphorescence.

5

45. The apparatus of claim 41, **characterized** in the apparatus further comprises third detector means arranged to detect radiation originating from evanescent wave stimulated scattering, particularly SPR-excited scattering.

- 10 46. A method of performing total internal reflection (TIR) based spectroscopy, which method comprises:
- irradiating at least one area of a plane surface (16; 36) of a transparent body (15; 35) with at least one collimated beam of electromagnetic radiation (19; 37) so that the radiation is totally internally reflected at the surface,
  - 15 imaging onto a respective two-dimensional detector array (D) at least one of (i) radiation internally reflected from the illuminated area or areas, (ii) fluorescent or phosphorescent radiation from the illuminated area or areas caused by evanescent wave stimulation, and (iii) radiation originating from evanescent wave stimulated scattering at the illuminated area or areas,
  - 20 sequentially or continuously scanning the incident angle over an angular range, the illuminated area or areas having an at least substantially fixed centre position during angular scan,
  - measuring at at least a number of incident angles of the radiation reflected at the surface of the transparent body, the intensities of the radiation imaged on different parts
  - 25 of the detector array (D), and
  - determining from the detected radiation intensities at the different incident angles at the transparent body surface, at least one of an optical thickness image, a refractive index image, a surface concentration image of the surface, and variation of such images with time,
  - 30 **characterized** by continuously varying the cross-sectional intensity of at least one of (i) the at least one beam of collimated electromagnetic radiation (19; 37) incident on the plane surface (16; 36) of the transparent body (15; 35), and (ii) the at least one beam of collimated electromagnetic radiation (19; 37) reflected from the plane surface

(16; 36) of the transparent body, in dependence of the incident angle at the surface during the angular scan to reduce variations of the irradiance in the illuminated area or areas of fixed centre position of the surface due to varying length extension in the plane of incidence of the illuminated surface area or areas during the angular scan, or the effect of such variation on the reflected beam or beams.

47. The method of claim 46, **characterized** by varying the cross-sectional intensity of the at least one beam of collimated electromagnetic radiation (19; 37) incident on the plane surface (16; 36) of the transparent body (15; 35).

10

48. The method of claim 46 or 47, **characterized** in that the method comprises varying the cross-sectional area's length of the at least one beam of collimated electromagnetic radiation (19; 37) in the plane of incidence at the at least one sensing surface in dependence of the incident angle during the angular scan.

15

49. The apparatus of claim 46 or 47, **characterized** in that the method comprises varying the power of the at least one beam of collimated electromagnetic radiation incident or reflected from the plane surface.

50. The apparatus of claim 49, **characterized** in that the power of the at least one beam is varied before scanning the beam.

51. The method of claim any one of claims 46 to 50 for performing ATR-spectroscopy, **characterized** in that radiation internally reflected from the illuminated area or areas is imaged on the detector array.

25

52. The method of any one of claims 46 to 51, **characterized** in that the method is performed at at least two different wavelengths.

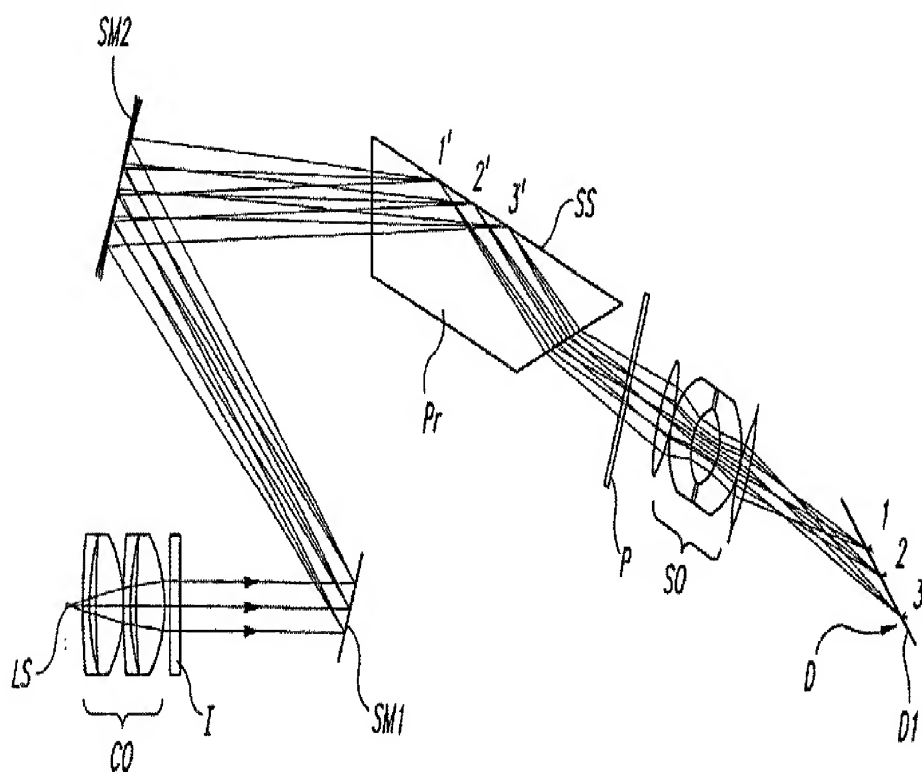


Fig. 1

PRIOR ART



2/5

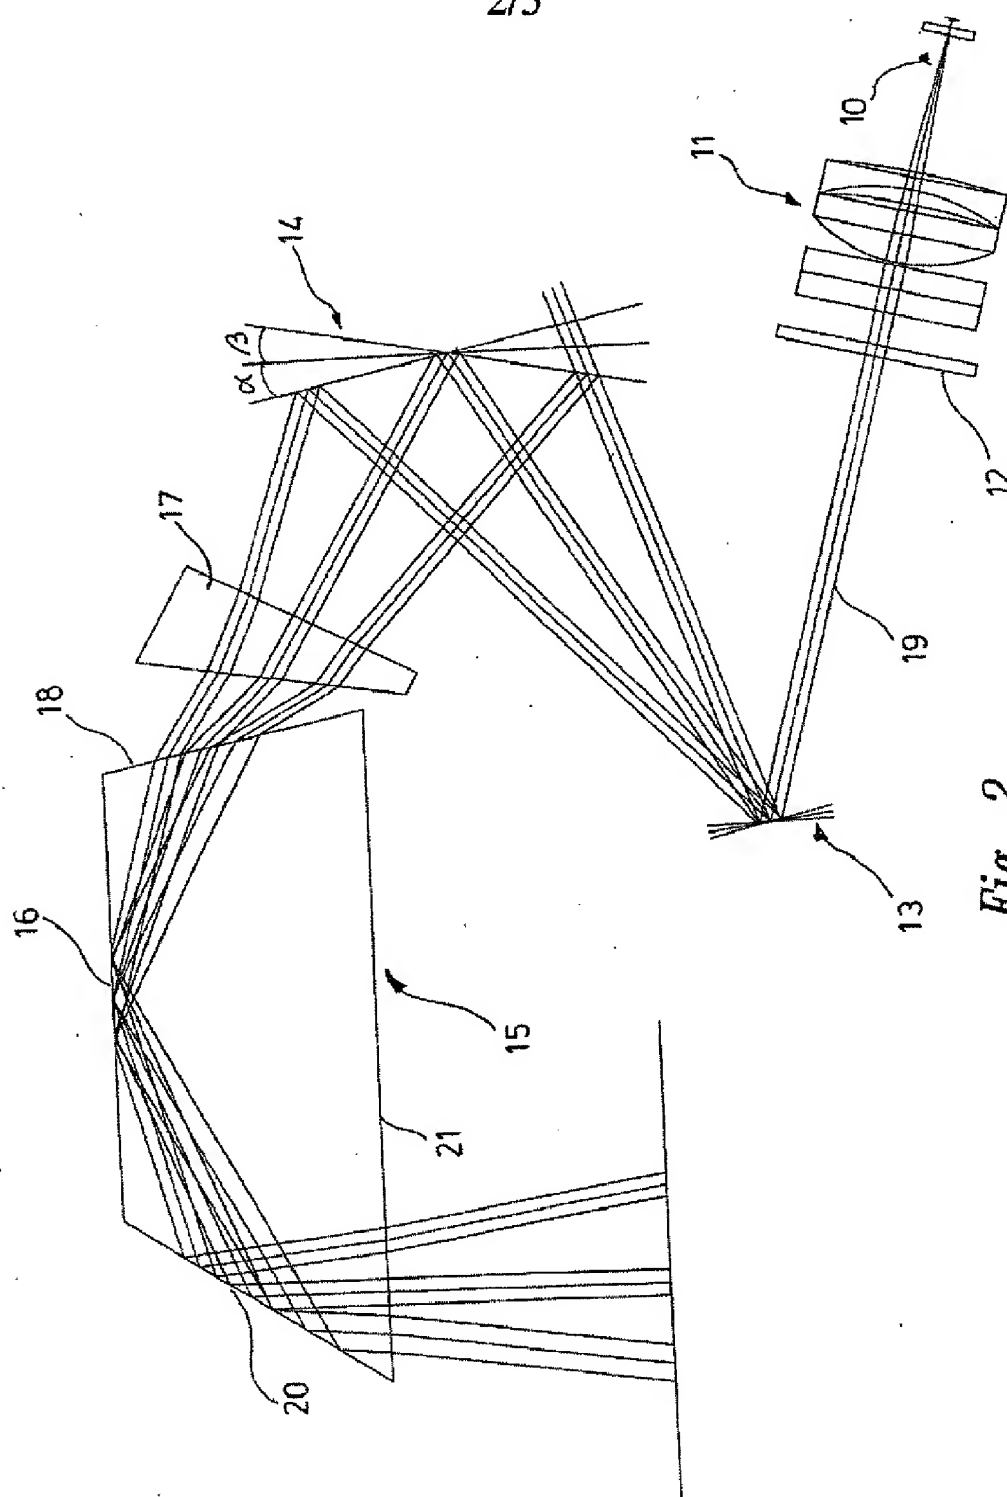
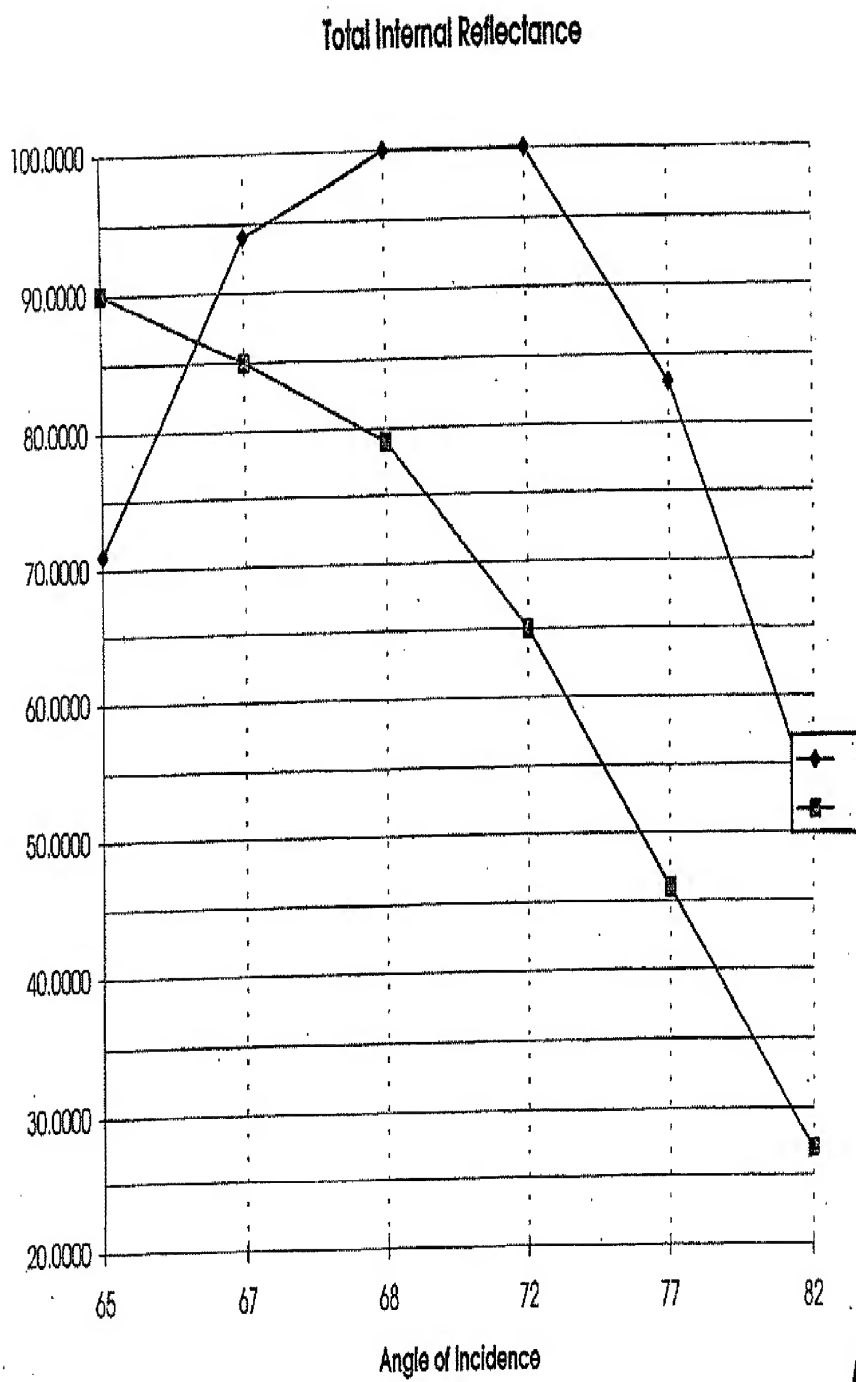


Fig. 2

*Fig. 3*

4/5

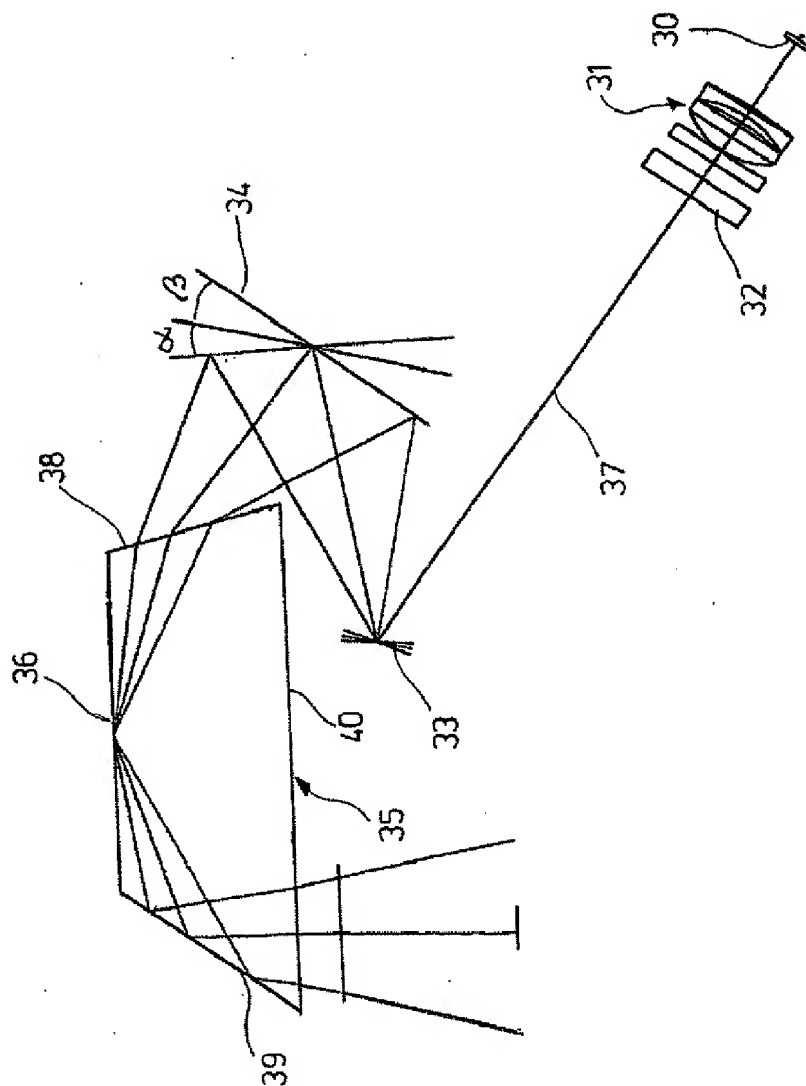


Fig. 4

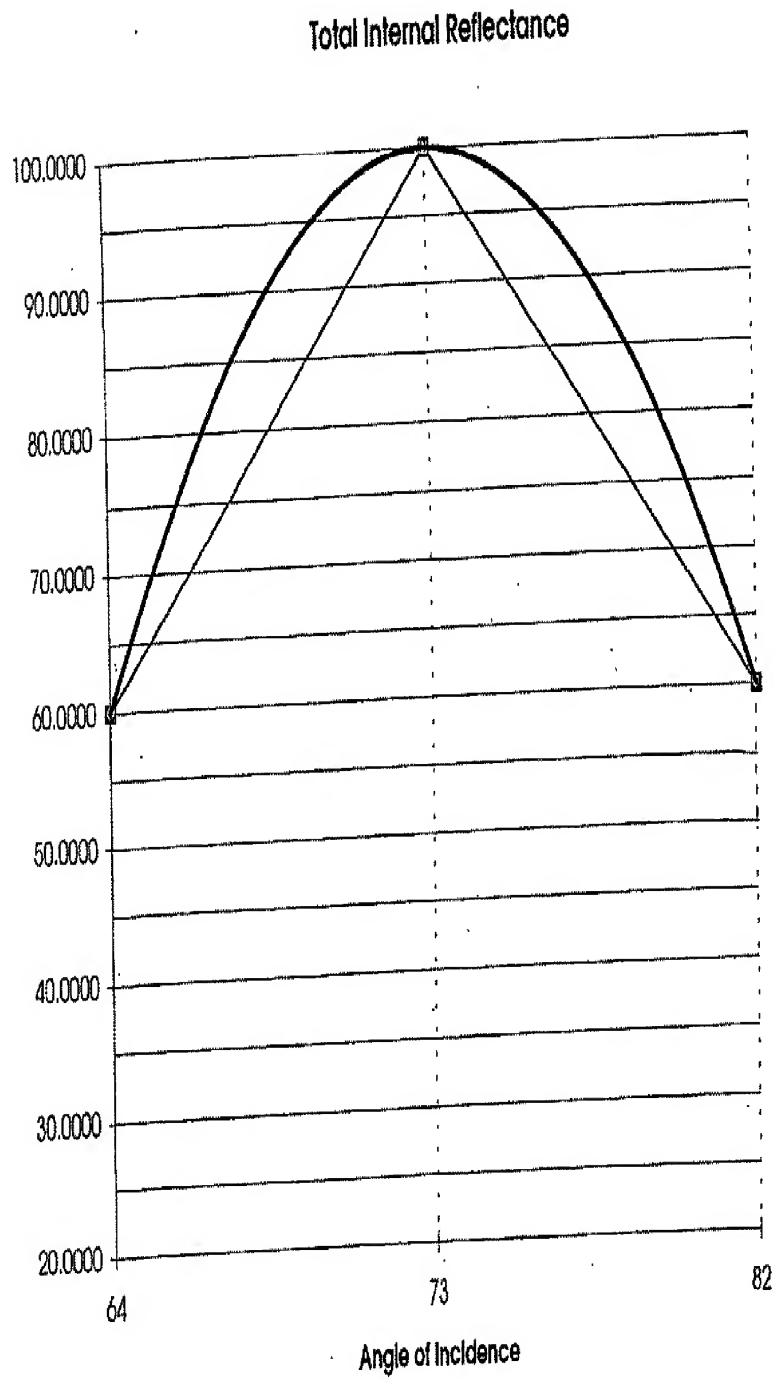


Fig. 5

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 02/00482

## A. CLASSIFICATION OF SUBJECT MATTER

IPC7: G01N 21/55

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: G01N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

EPODOC,WPI,PAJ,IEC

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
Y	WO 9834098 A1 (BIACORE AB SE), 6 August 1998 (06.08.98), figure 1, claims --	1-52
Y	JP 4-15976 A (MITSUI PETROCHEM IND LTD), 21 January 1992 (21.01.92), figure 12 --	1-52
P,A	JP 2001-188023 A (YOKOGAWA ELECTRIC CORP), 10 July 2001 (10.07.01), figure 10 --	1-52
A	WO 9822808 A1 (THE SECRETARY OF STATE FOR DEFENCE GB), 28 May 1998 (28.05.98), page 5, line 19 - line 26 --	1-52



Further documents are listed in the continuation of Box C.



See patent family annex.

\*

Special categories of cited documents:

"A"

document defining the general state of the art which is not considered to be of particular relevance

"E"

earlier application or patent but published on or after the international filing date

"L"

document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)

"O"

document referring to an oral disclosure, use, exhibition or other means

"P"

document published prior to the international filing date but later than the priority date claimed

"T"

later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention

"X"

document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone

"Y"

document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art

"&amp;"

document member of the same patent family

Date of the actual completion of the international search

17 June 2002

Date of mailing of the international search report

27 -06- 2002

Name and mailing address of the ISA/

Swedish Patent Office

Box 5055, S-102 42 STOCKHOLM

Facsimile No. +46 8 666 02 86

Authorized officer

Sture Elnäs/itw

Telephone No. +46 8 782 25 00

## INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 02/00482

## C (Continuation). DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	WO 9425850 A1 (FISONS PLC), 10 November 1994 (10.11.94), page 10, line 6 - line 14  --	1-52
A	WO 9205426 A1 (AMERSHAM INTERNATIONAL PLC), 2 April 1992 (02.04.92), figure 9, abstract  -----	1-52

INTERNATIONAL SEARCH REPORT  
Information on patent family members

01/05/02

International application No.

PCT/SE 02/00482

Patent document cited in search report			Publication date	Patent family member(s)		Publication date
WO	9834098	A1	06/08/98	AU	719654 B	11/05/00
				AU	1950497 A	22/09/97
				AU	5893198 A	25/08/98
				EP	0958494 A,B	24/11/99
				JP	2001511249 T	07/08/01
				SE	9700384 D	00/00/00
-----						
JP	4-15976	A	21/01/92	NONE		
-----						
JP	2001-188023	A	10/07/01	NONE		
-----						
WO	9822808	A1	28/05/98	AU	737114 B	09/08/01
				AU	4875297 A	10/06/98
				CN	1244919 A	16/02/00
				EP	0938661 A	01/09/99
				GB	9623820 D	00/00/00
				IL	129923 D	00/00/00
				JP	2001504582 T	03/04/01
				NO	992326 A	16/07/99
				TW	400432 B	00/00/00
				US	6268125 B	31/07/01
				US	2002016011 A	07/02/02
ZA	9709734 A	22/05/98				
-----						
WO	9425850	A1	10/11/94	GB	9308728 D	00/00/00
-----						
WO	9205426	A1	02/04/92	EP	0548215 A	30/06/93
				GB	9019999 D	00/00/00
-----						